


# Installation and Test Procedures for the CM-9201 ESD Monitor

1. Mount the CM-9201 in a convenient place on the workbench using the screws supplied with the unit or the optional mounting bracket. Units are frequently mounted on the underside of the workbench to keep them out of the way.
2. Plug the power adaptor into the CM-9201 and into a grounded outlet. The LED should turn red and the buzzer should sound. The ground in the outlet is an important part of the system and should be also connected to the ESD Common Point Ground.
3. Plug a wrist strap into the front of the unit and put it on. The OPERATOR LED should turn green. If it doesn't, touch the wrist strap to the common point ground. If the turns green, then the wrist strap was not making good contact with the OPERATOR. The outlet and the Common Point Ground can located at any convenient place on the workbench. OPERATOR

## Connection Diagram

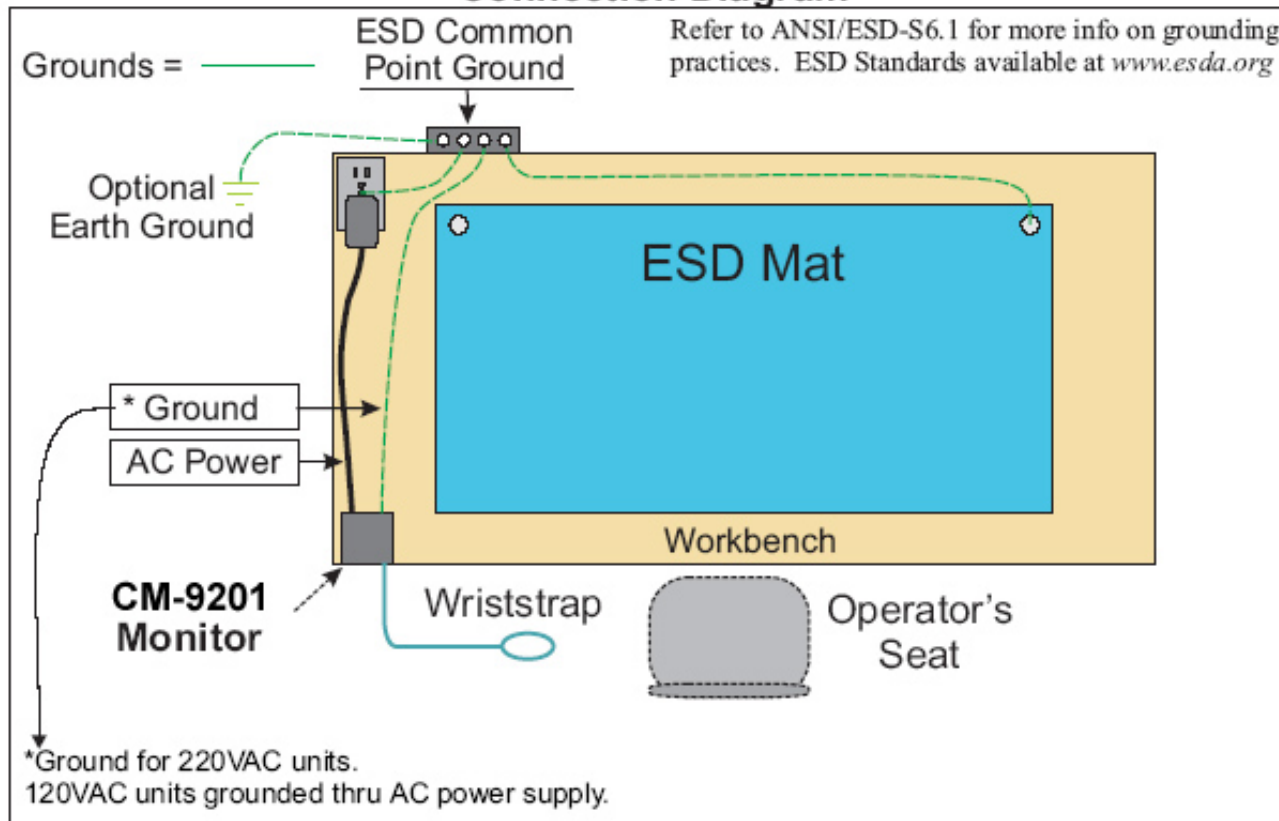

The **CM-9201-TM** Calibration and Test unit is available for the CM-9201. Plug the ground cable into the Common Point Ground and the Operator cable into the OPERATOR input. The LED should be red. It should turn green when you press the test button.

## CM-9201 INSTALLATION & TEST PROCEDURES

PRODUCT  
CM-9201

ITEM NUMBER  
CM-9201

DATA SHEET



1-877-GND-ZERO (463-9376)  
FAX: 941-751-7586  
4916 26<sup>TH</sup> Street West #100  
Bradenton, Florida 34207  
EMAIL: [sales@gndzero.com](mailto:sales@gndzero.com)  
[www.gndzero.com](http://www.gndzero.com)